

FORMED 163020-163020

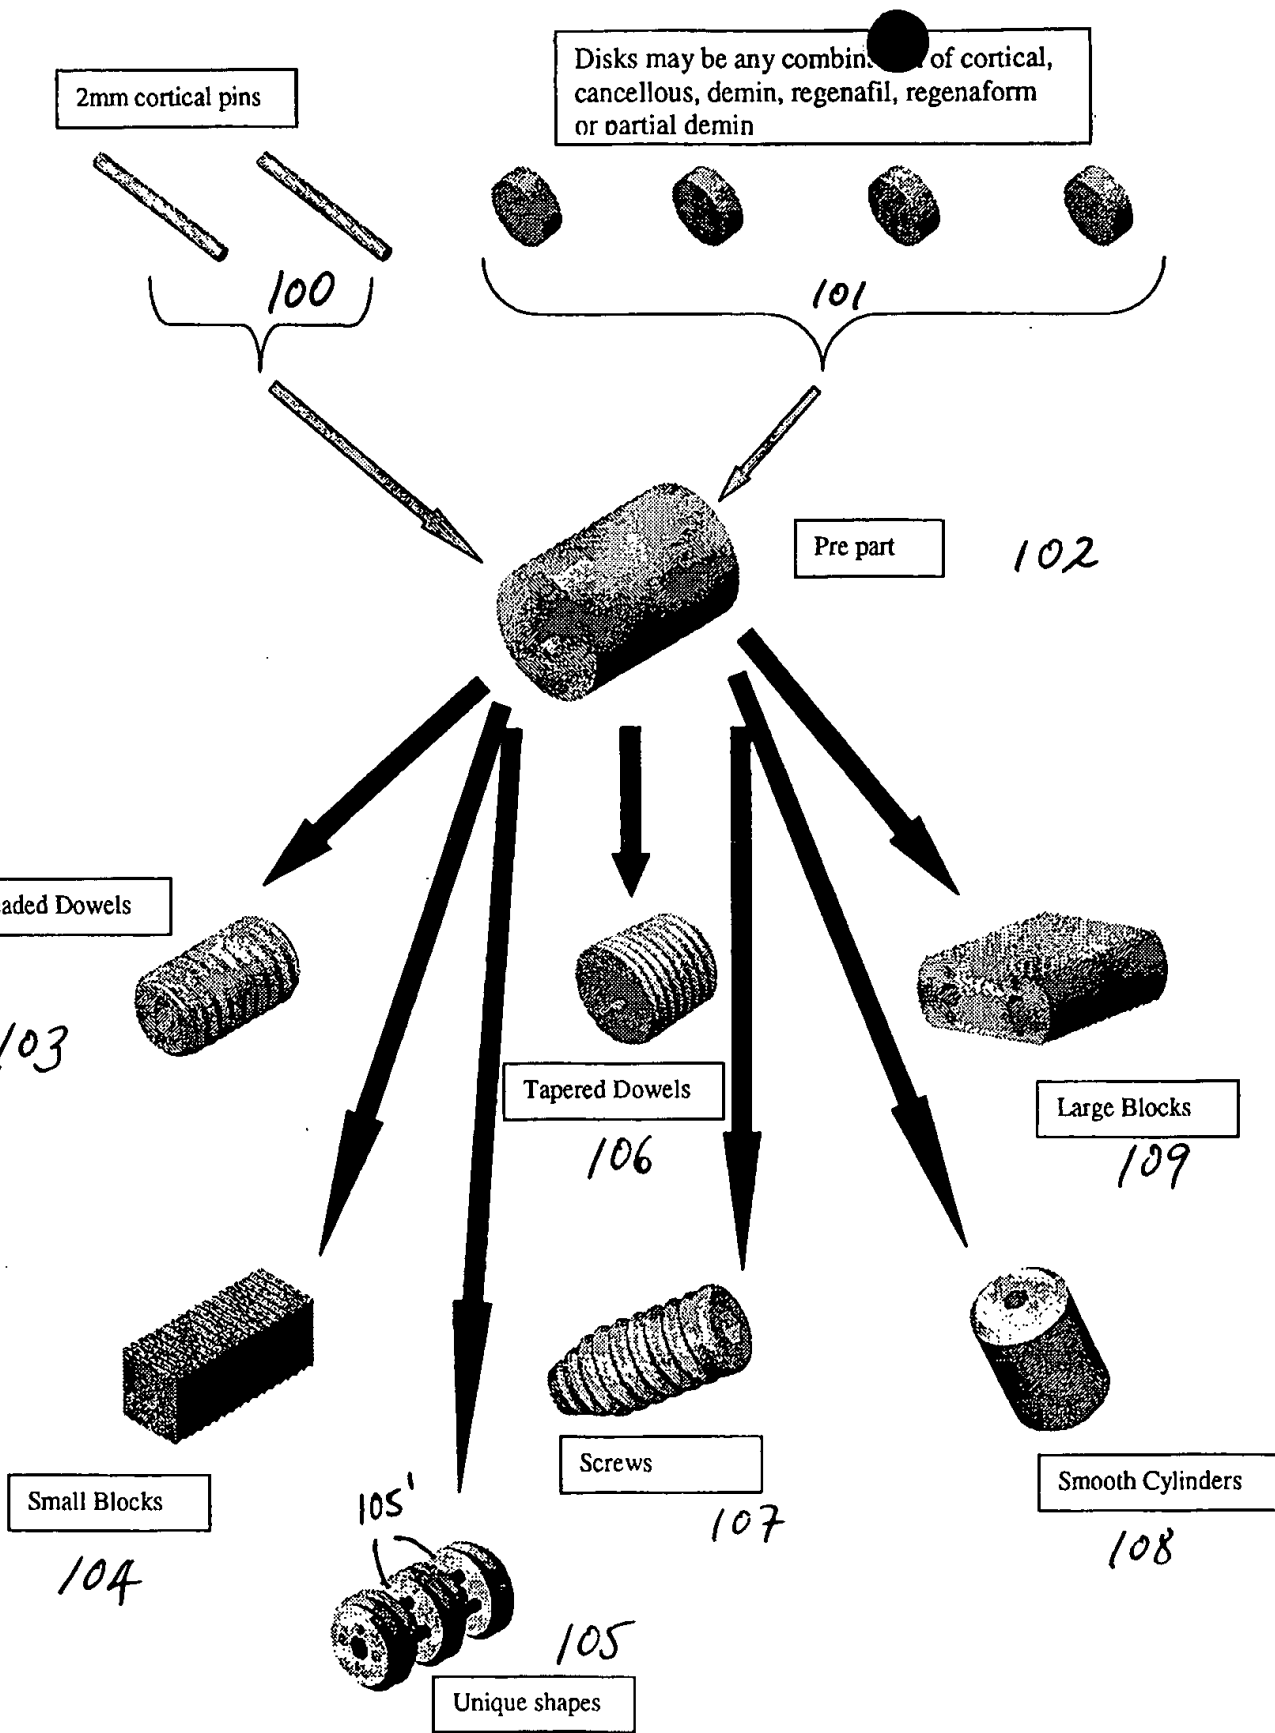


Figure 1

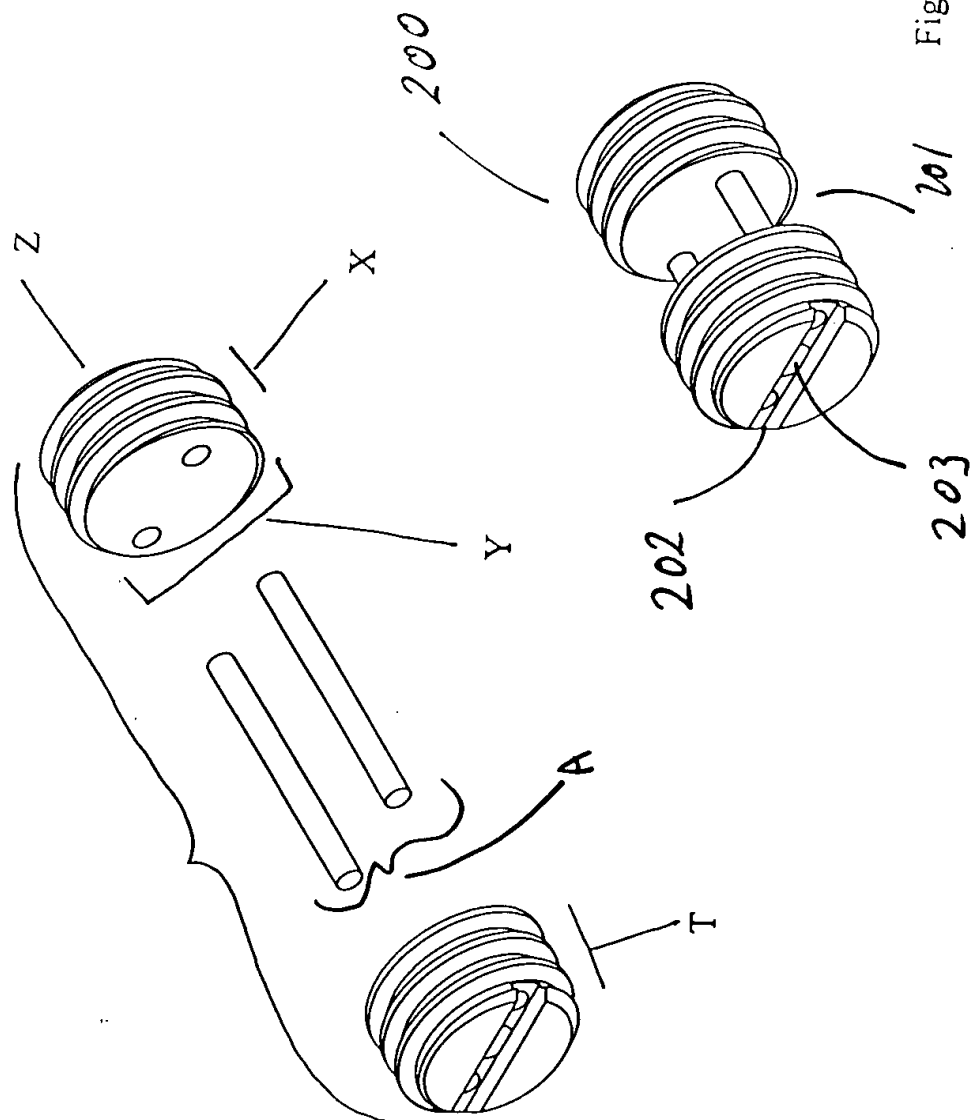


Figure 2

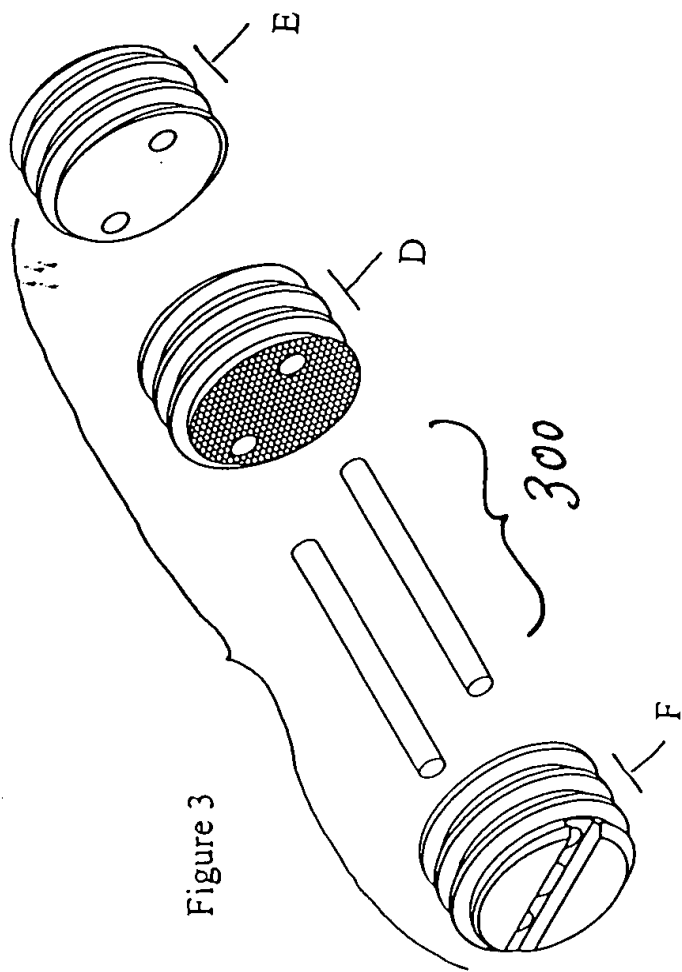


Figure 3

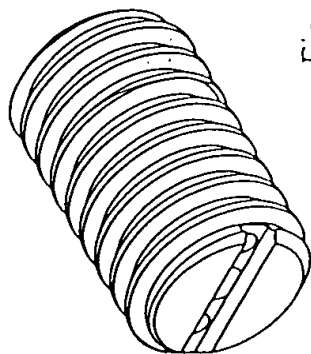


Figure 4

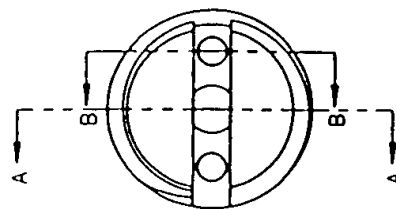


Figure 5

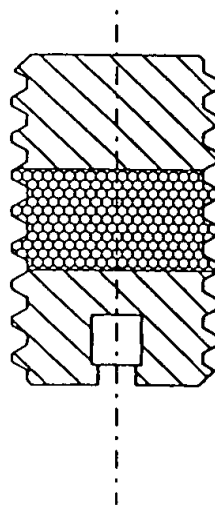


Figure 6

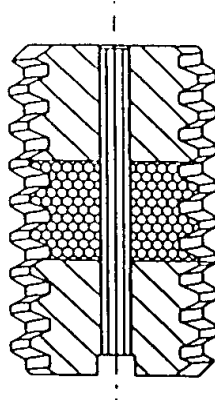


Figure 7

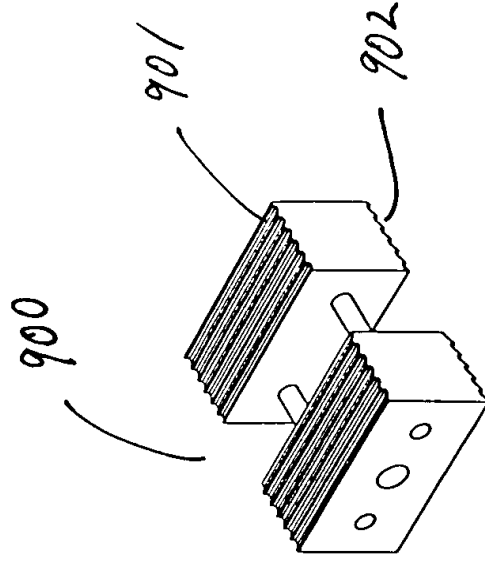
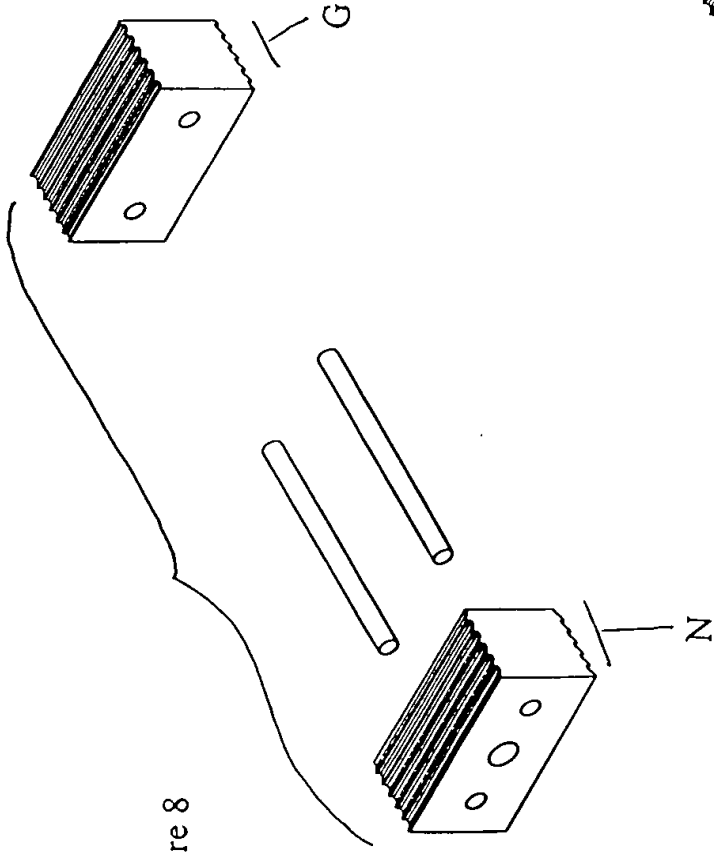


Figure 10

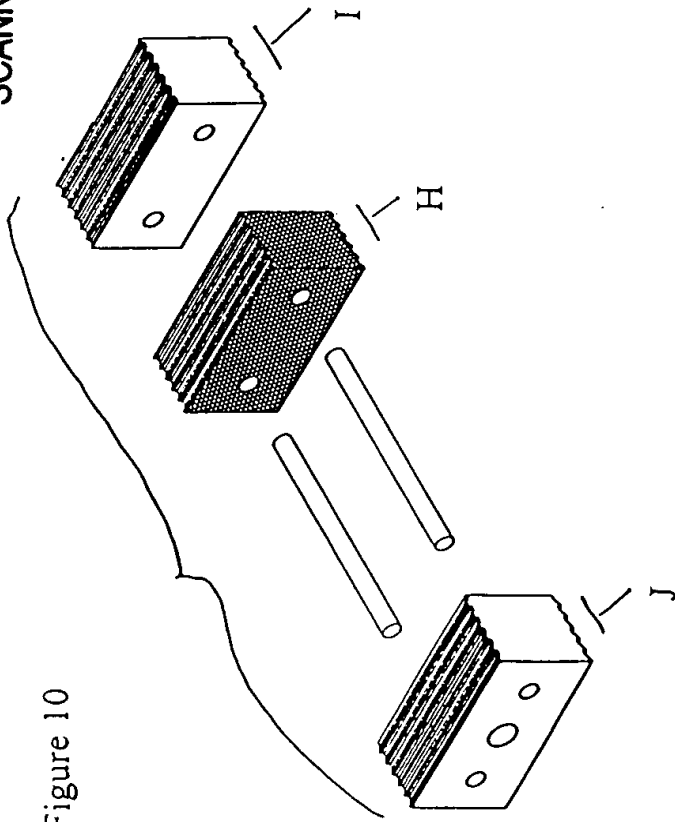


Figure 11

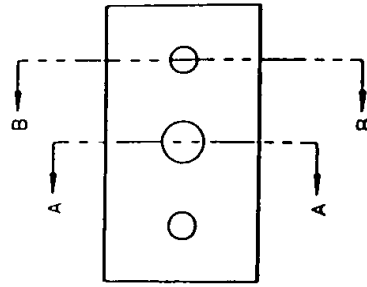
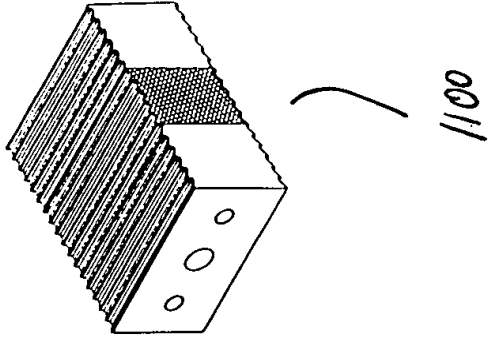


Figure 12

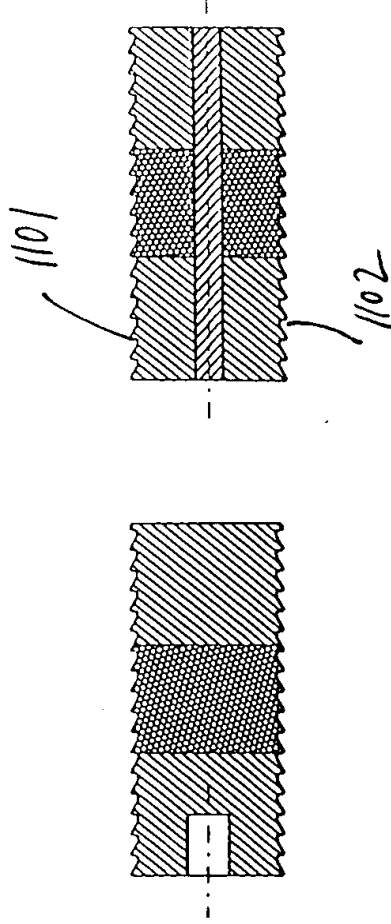


Figure 13

Figure 14

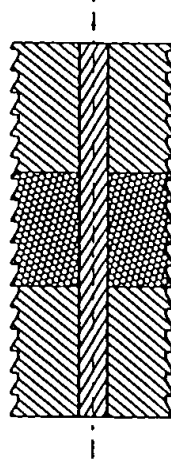
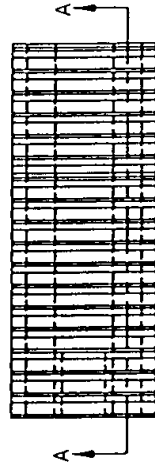
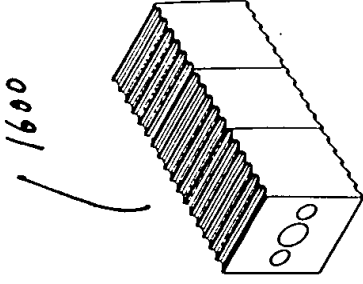
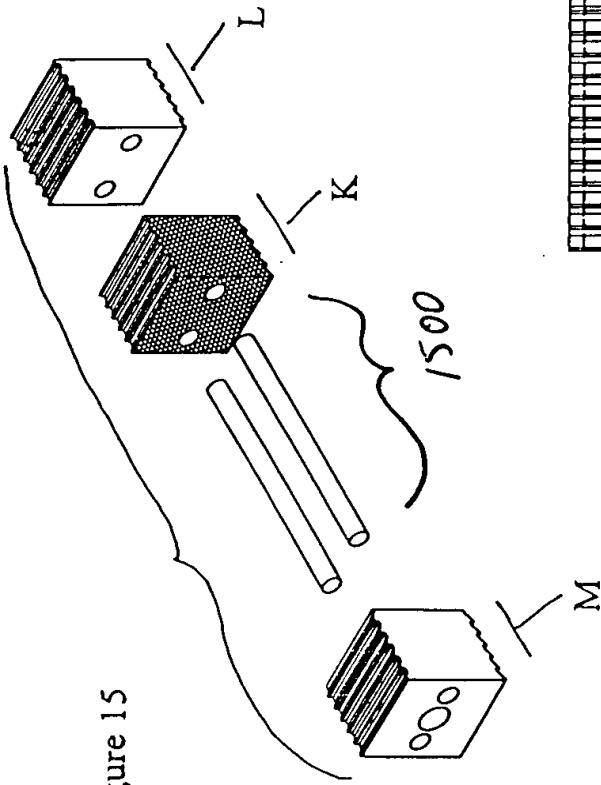


Figure 17

Figure 18

09783504.024304  
FOI 2010528600

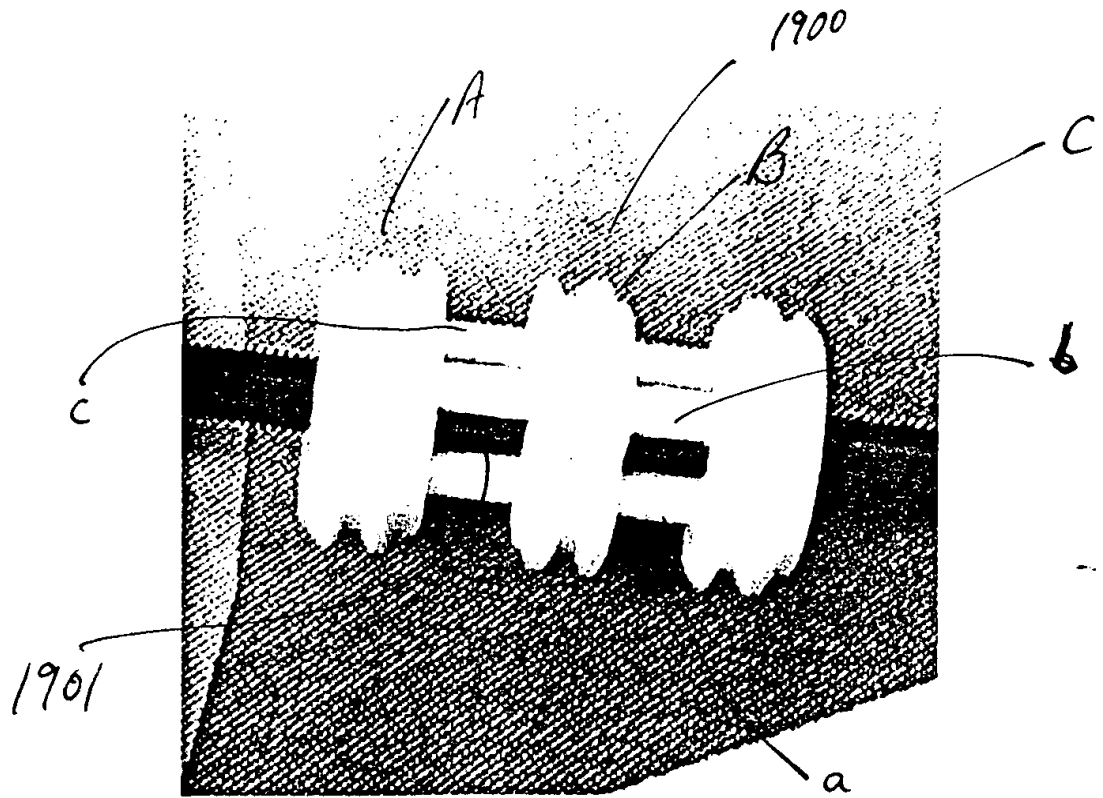


FIGURE 19

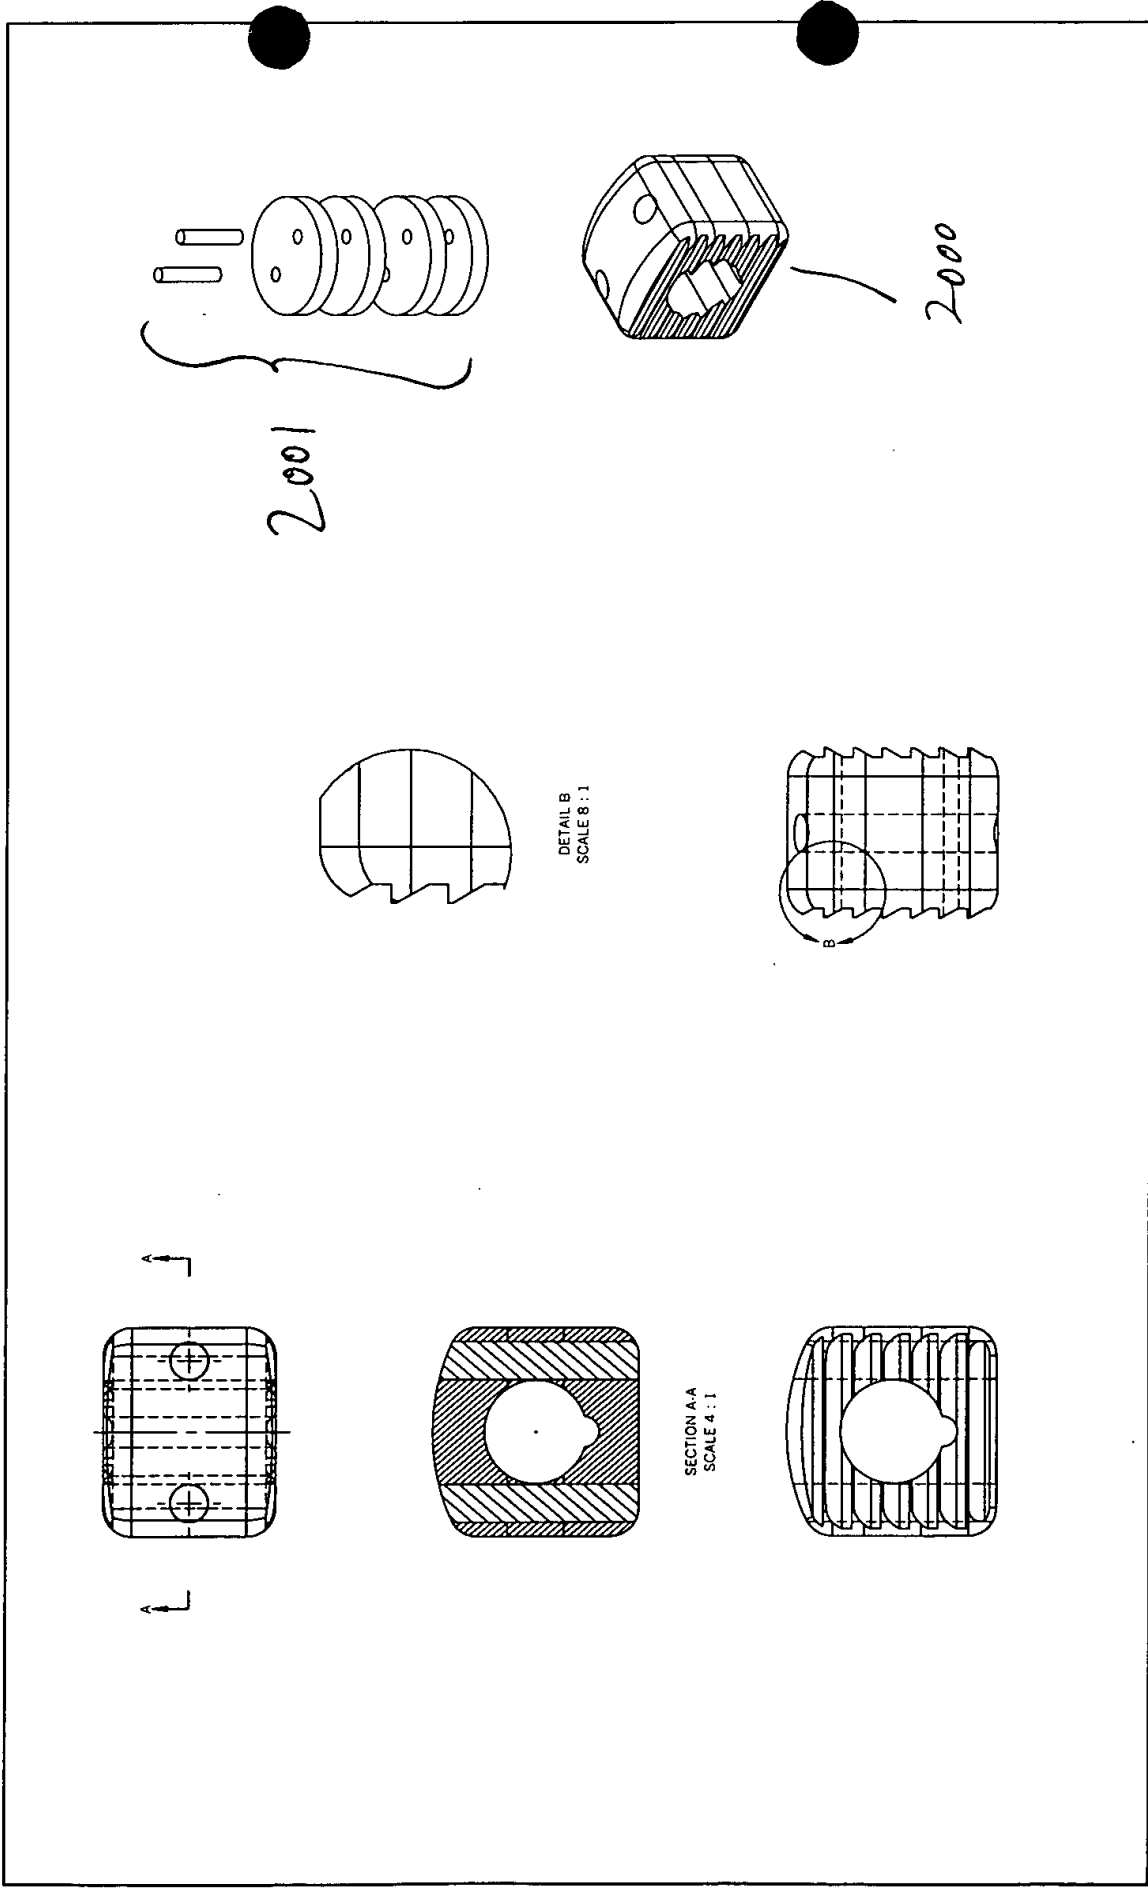


Figure 20





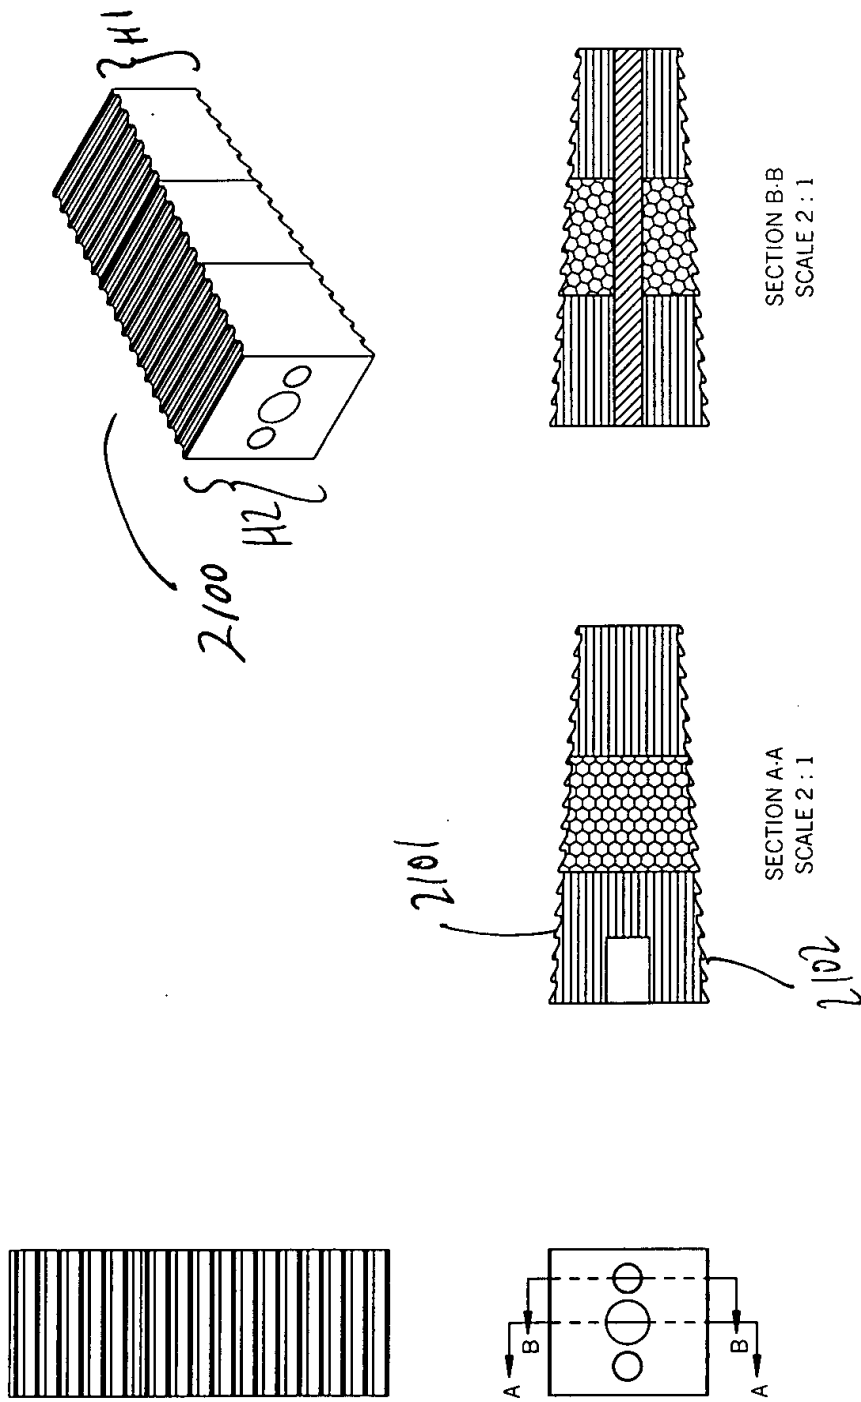


Figure 12

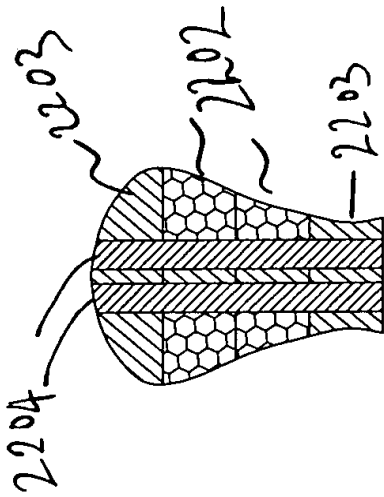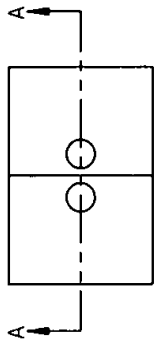

SECTION A-A  
SCALE 2 : 1




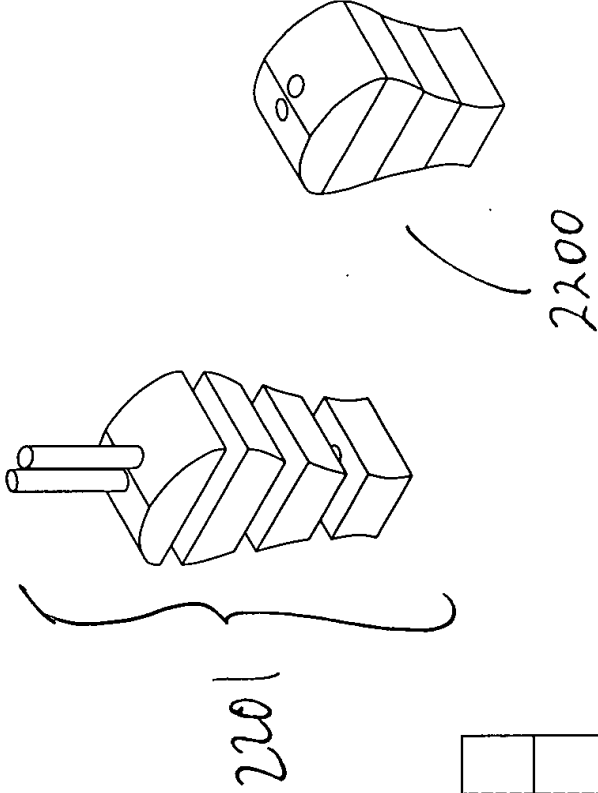


Figure 23

Create a tapered dowel!

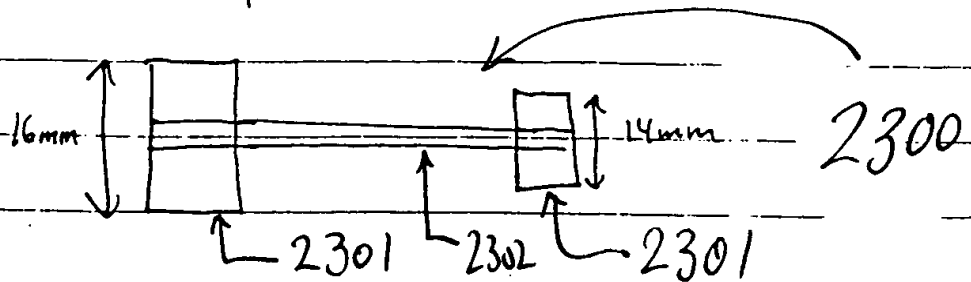

Salvage dowel out of spec

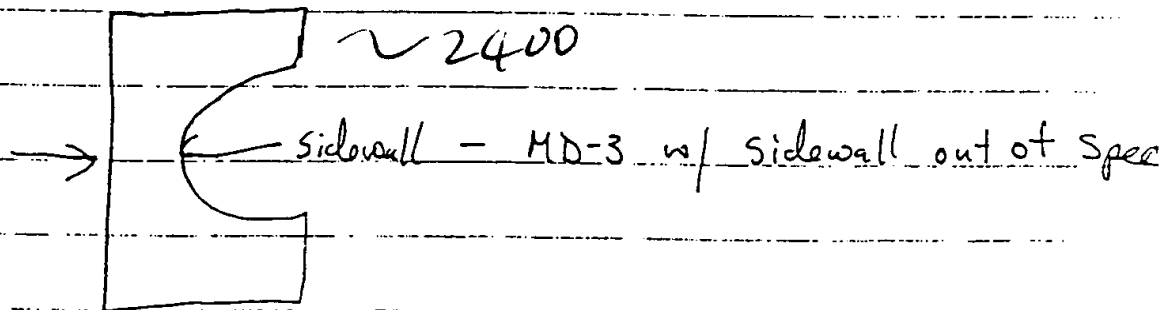

Solution - Create an MD-2

Figure 24A


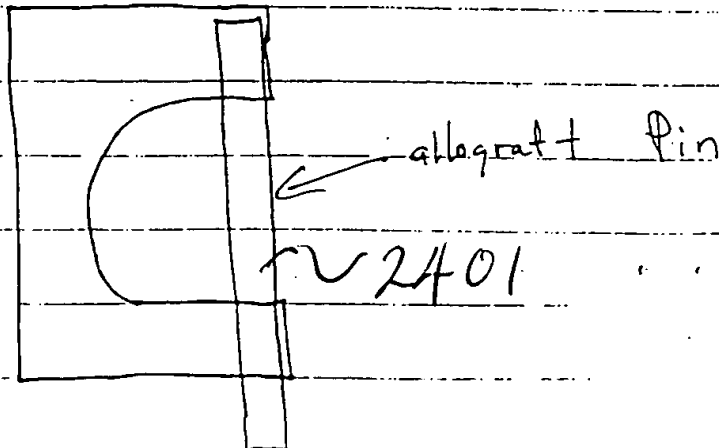



Figure 24B

Figure 24

Figure 25

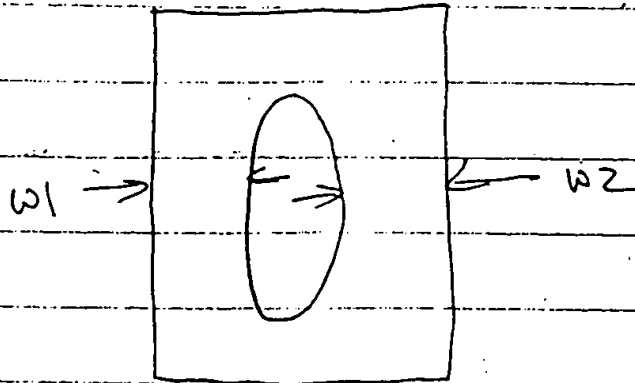


MD-2 out of spec @ Sidewall

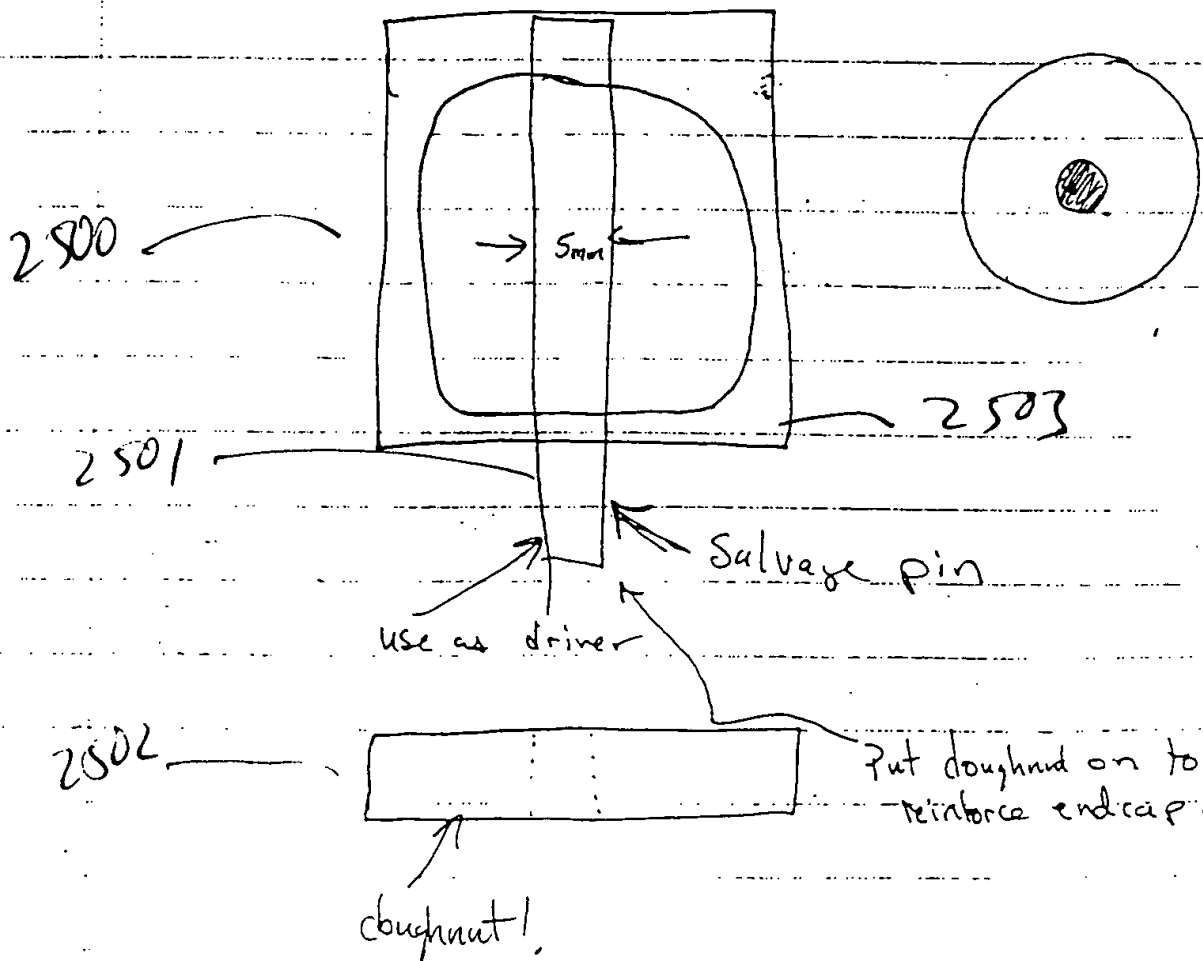


SCANNED, #12  
Figure 26

Cancellous bone


2600




12 x 2mm




6 x 2mm




9 x 3mm



12 x 3mm



6 x 3mm



6 x 4mm

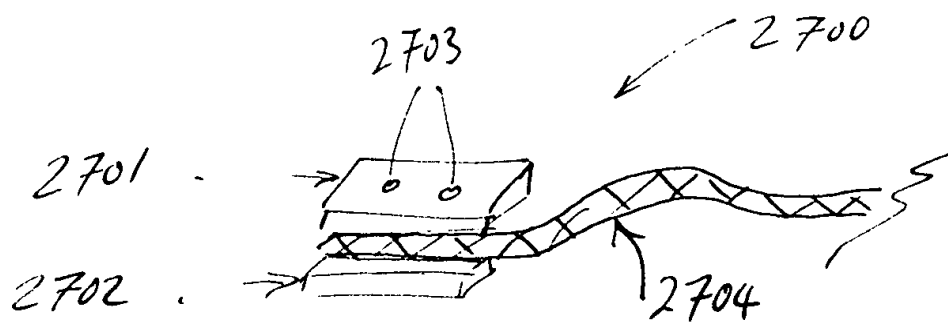


Figure 27

FIG. 27